

Introduction

This Test Interface is a hand held test clip, designed to probe simultaneously the leads of an assembled IC. Terminated with six 25 way male "D" type connectors, the interface makes temporary electrical contact with the leads of the device, in a two step action:

- the interface is positioned over the device leads (from underside the PCB) to be tested
 (lining up the test interface pins with the leads of the device that protrude through the PCB)
- by pushing the handle further, reliable contact will be made.

Features

- achieves the best combination of reliability, repeatability, serviceability and user-friendliness;
- high contact pressure at probe tip, for repeatable and reliable contact;
- high reliability and long life interchangeable microprobes;
- sweeping action gold plated contacts, for reliable contact and low ohmic resistance of interconnections;
- high current rating (for single channel, in ambient air with 70°F [20°C]) : 1.5A
- impact, solvent and temperature resistant plastics, with low friction;
- wide range of operating temperatures (commercial): [0°C to +70°C]
- clear markings on the body, indicating Pin 1 of IC being tested, to prevent probing the wrong way round;
- packaged in a hard wearing, high resistance to damage Polypropylene case with foam insets, the Test Interface can withstand high impact in transit.
- case can be used for safe storage when the Test Interface is not in use, and subsequent transport.



Specification


- It will accommodate a 132Pin HD PGA Footprint as detailed below;
- Maximum number of interconnections (channels): 132
- Current rating, with all contacts loaded (maximum continuous current, non inductive): 0.5A /channel;
- Contact resistance (average): 80 m Ω /channel;
- Insulation resistance: 5M Ω Min.
- Volume resistivity of plastic parts : 10^{15} Ω -cm @ 50%RH.
- Fatigue life of probes: Min. 1,000,000 cycles at normal working distance;
- Working distance (normal stroke): 1.8mm;
- Probe force at point of contact (normal stroke): 1.1N

Connections Table


Pin tables for this clip are available electronically:

- for Diagnosys employee's go to the R&D section on the Diagnosys intranet.
- for customers please contact Diagnosys sales.

HD PGA FOOTPRINT

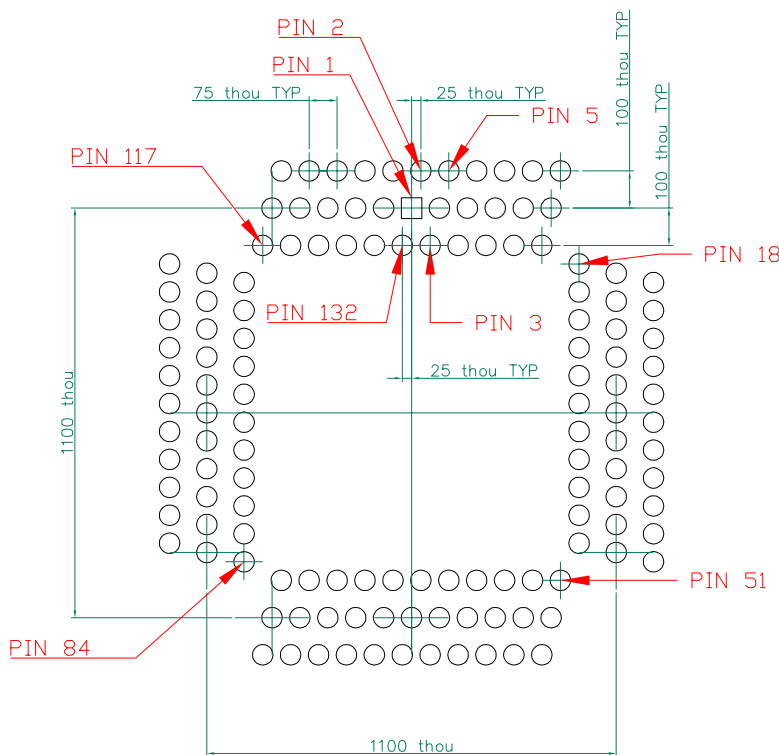

PCB UNDERSIDE VIEW

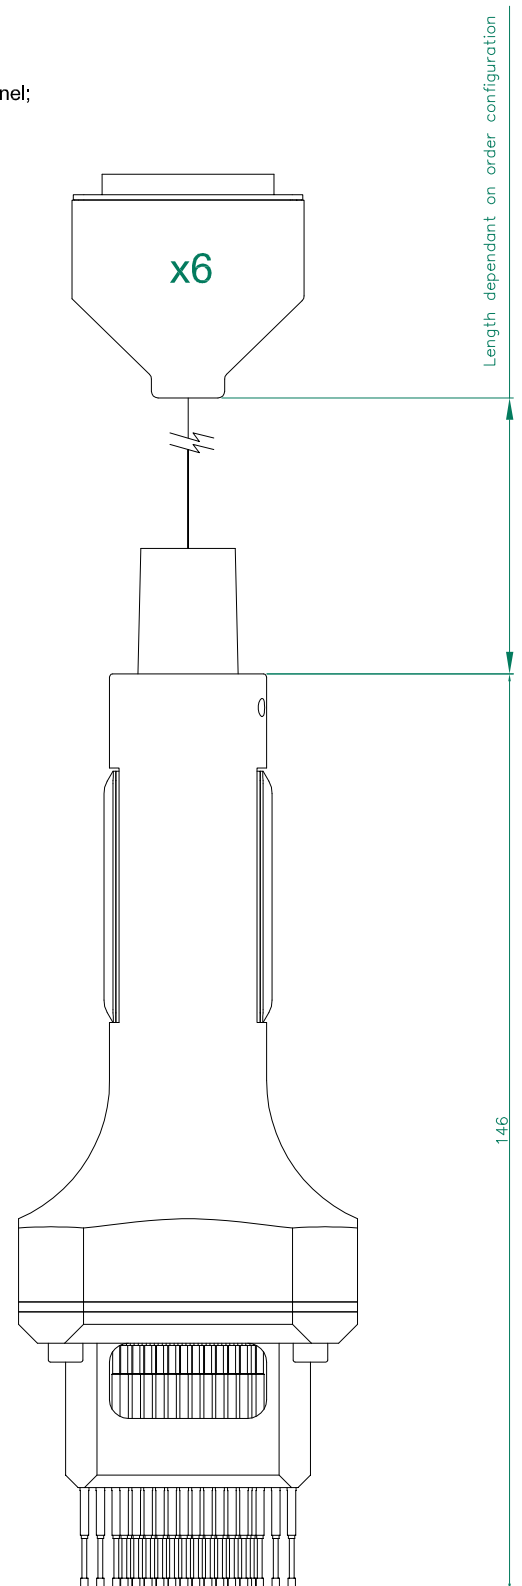

Maintenance

The Test Interface Head is maintenance free. The probes are self-cleaning. Immersion in water or contact between probes and any liquids should be avoided, as this could severely reduce the working life of microprobes.

Contamination is the primary cause of probe contact problems. This is generally caused by flux left as a residue on circuit boards. Other probe contaminants such as dust, fluff, oil and grime can also cause problems in other areas. Light brushing of the tips of the probes with nylon, bristle or soft metal brushes will dislodge most contaminants.